

123

102

180-

106

Fig. 1

Analyzer
175

FIG. 2

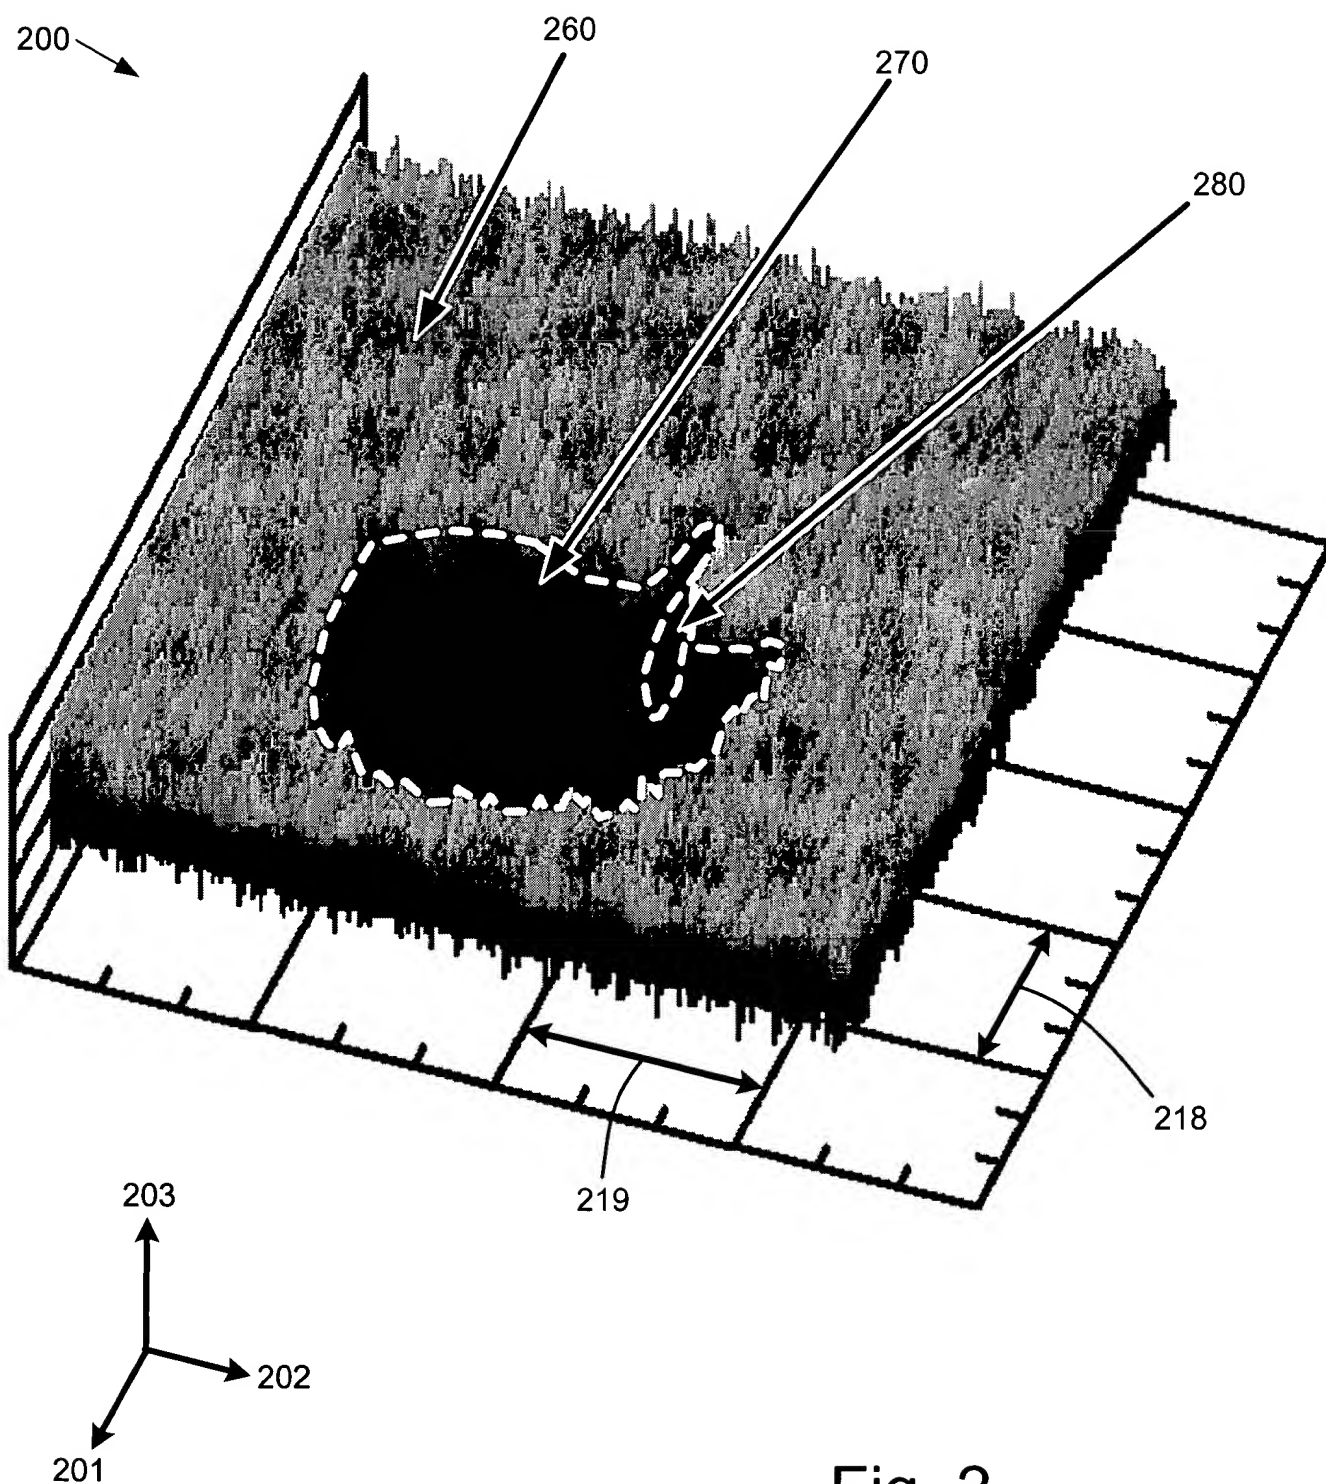


Fig. 2

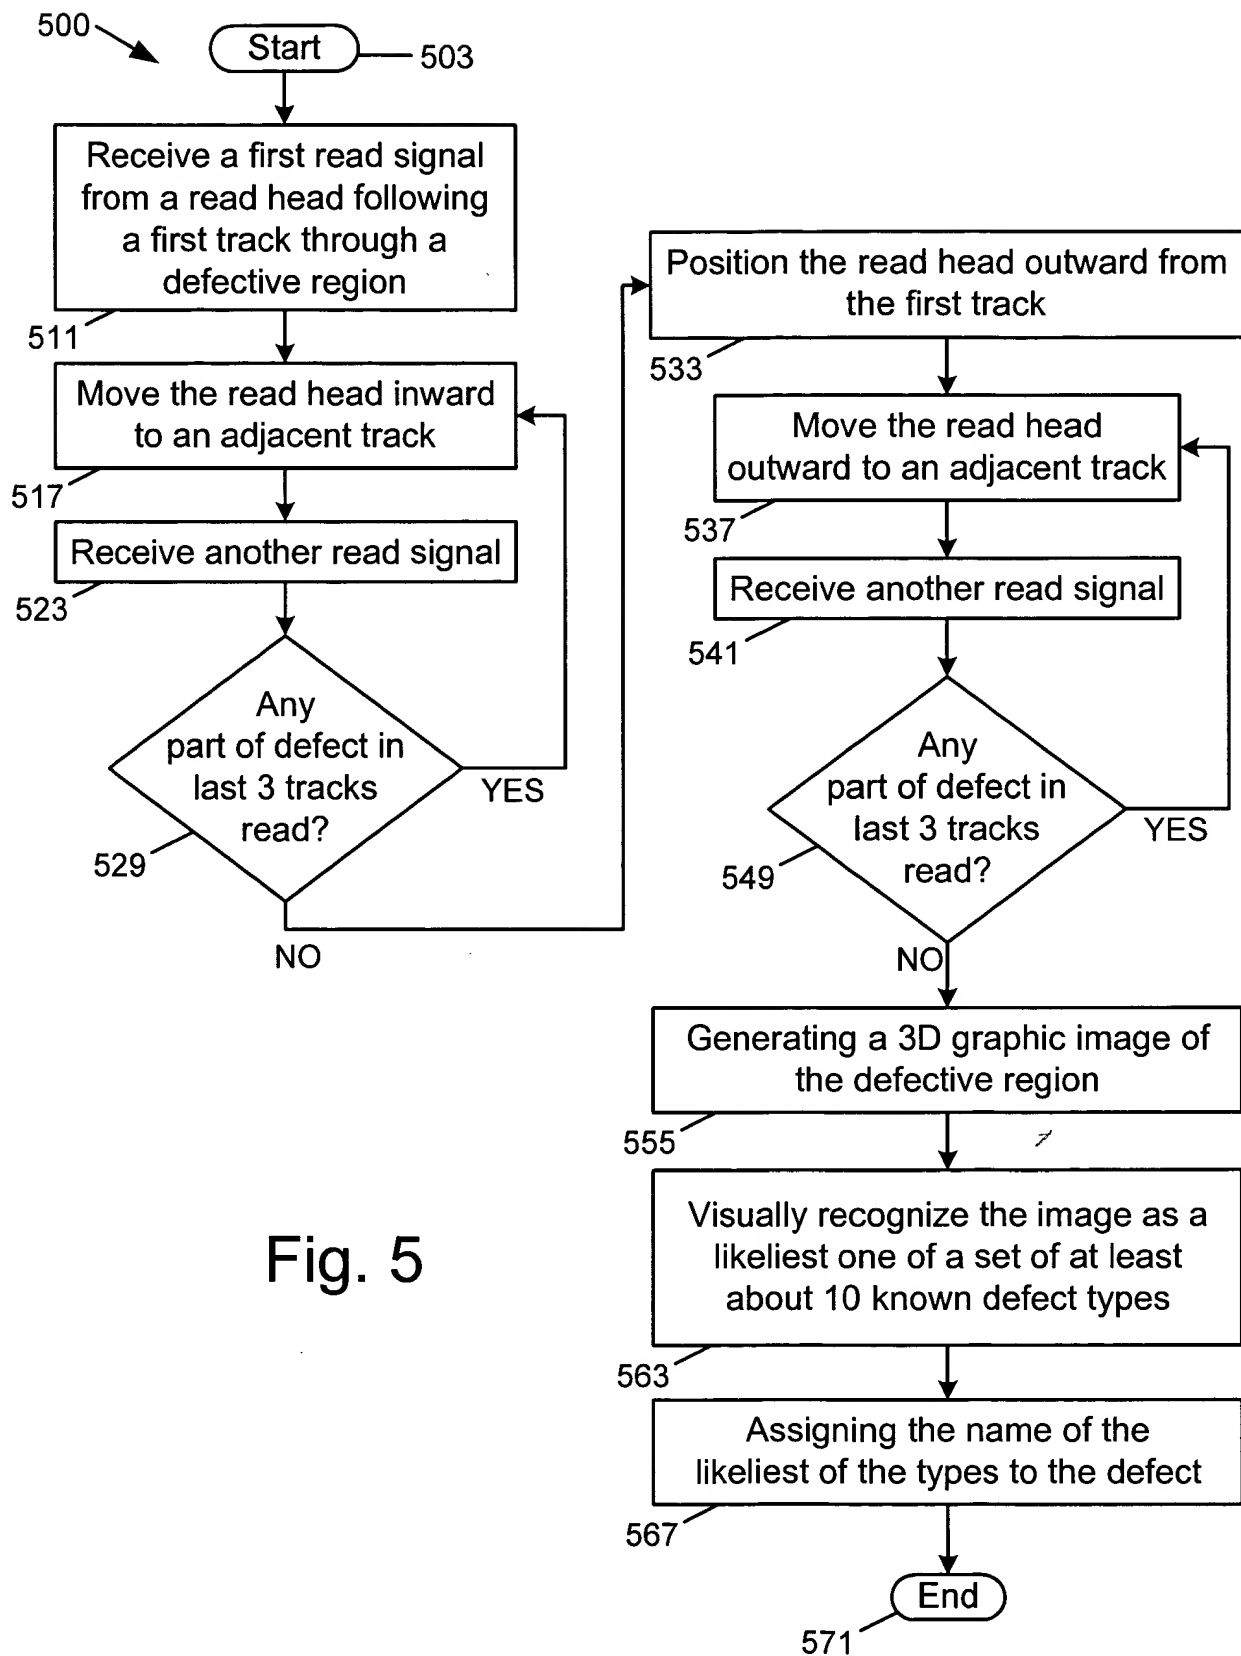


Fig. 5

FIG. 5

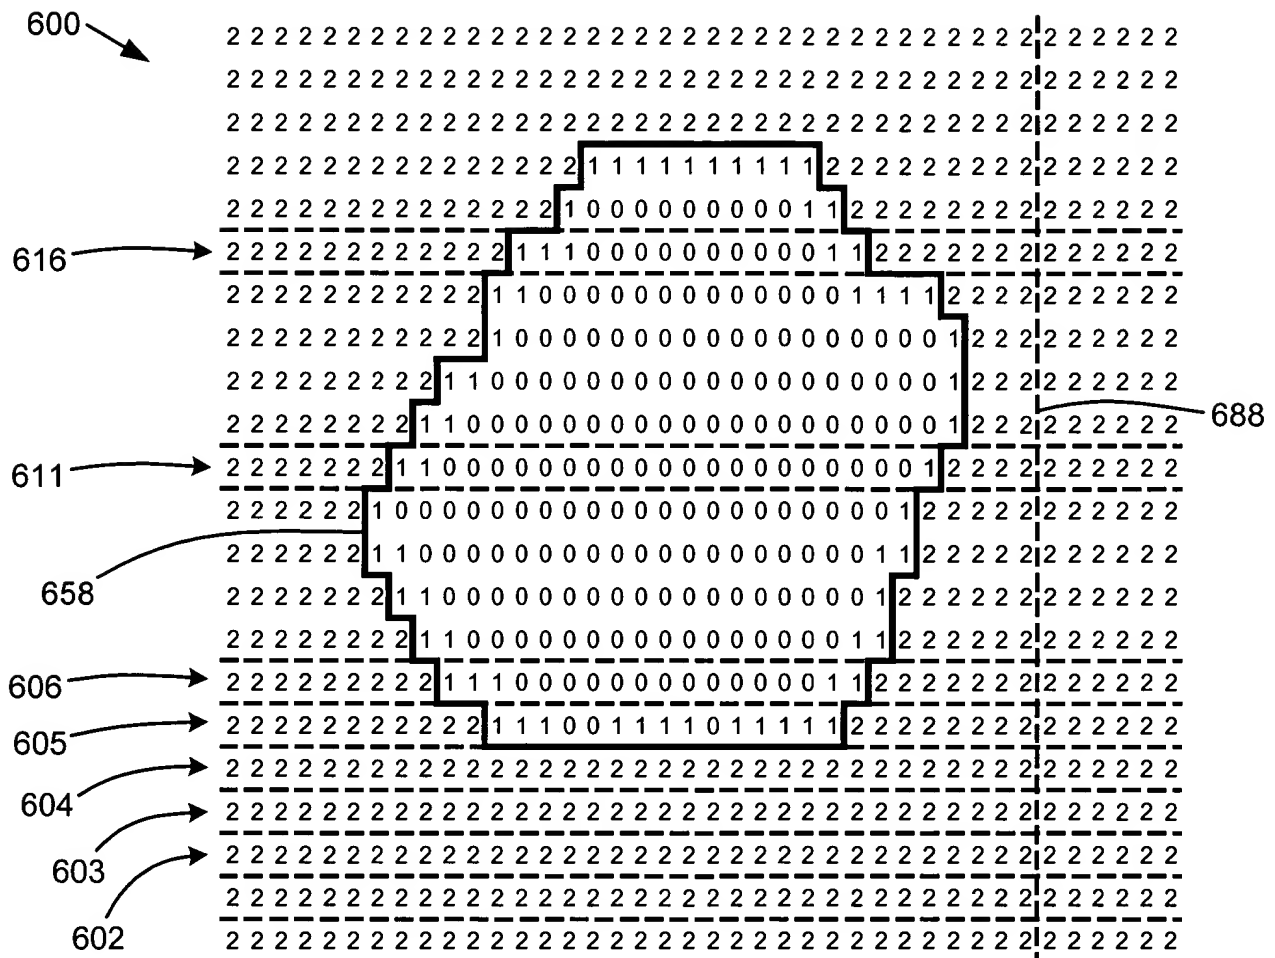


Fig. 6


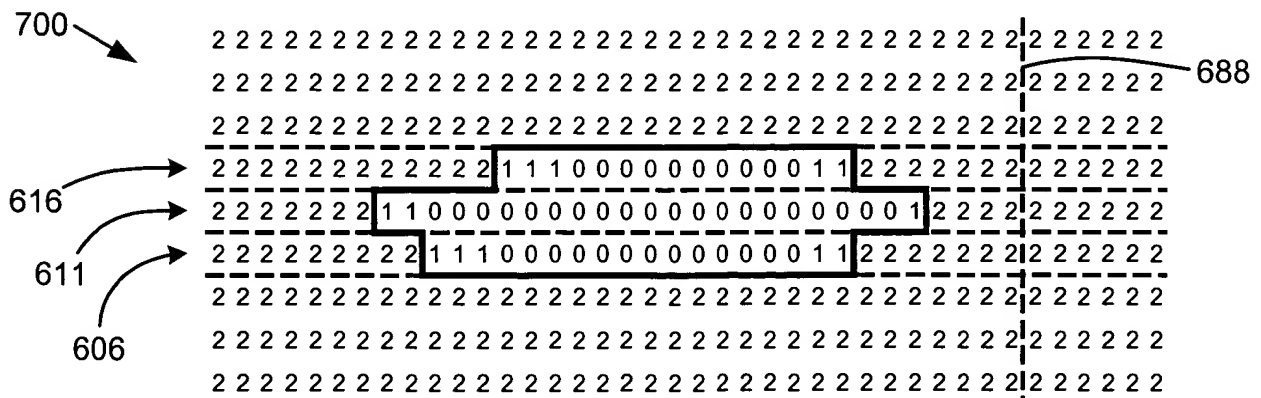


Fig. 7

Fig. 8

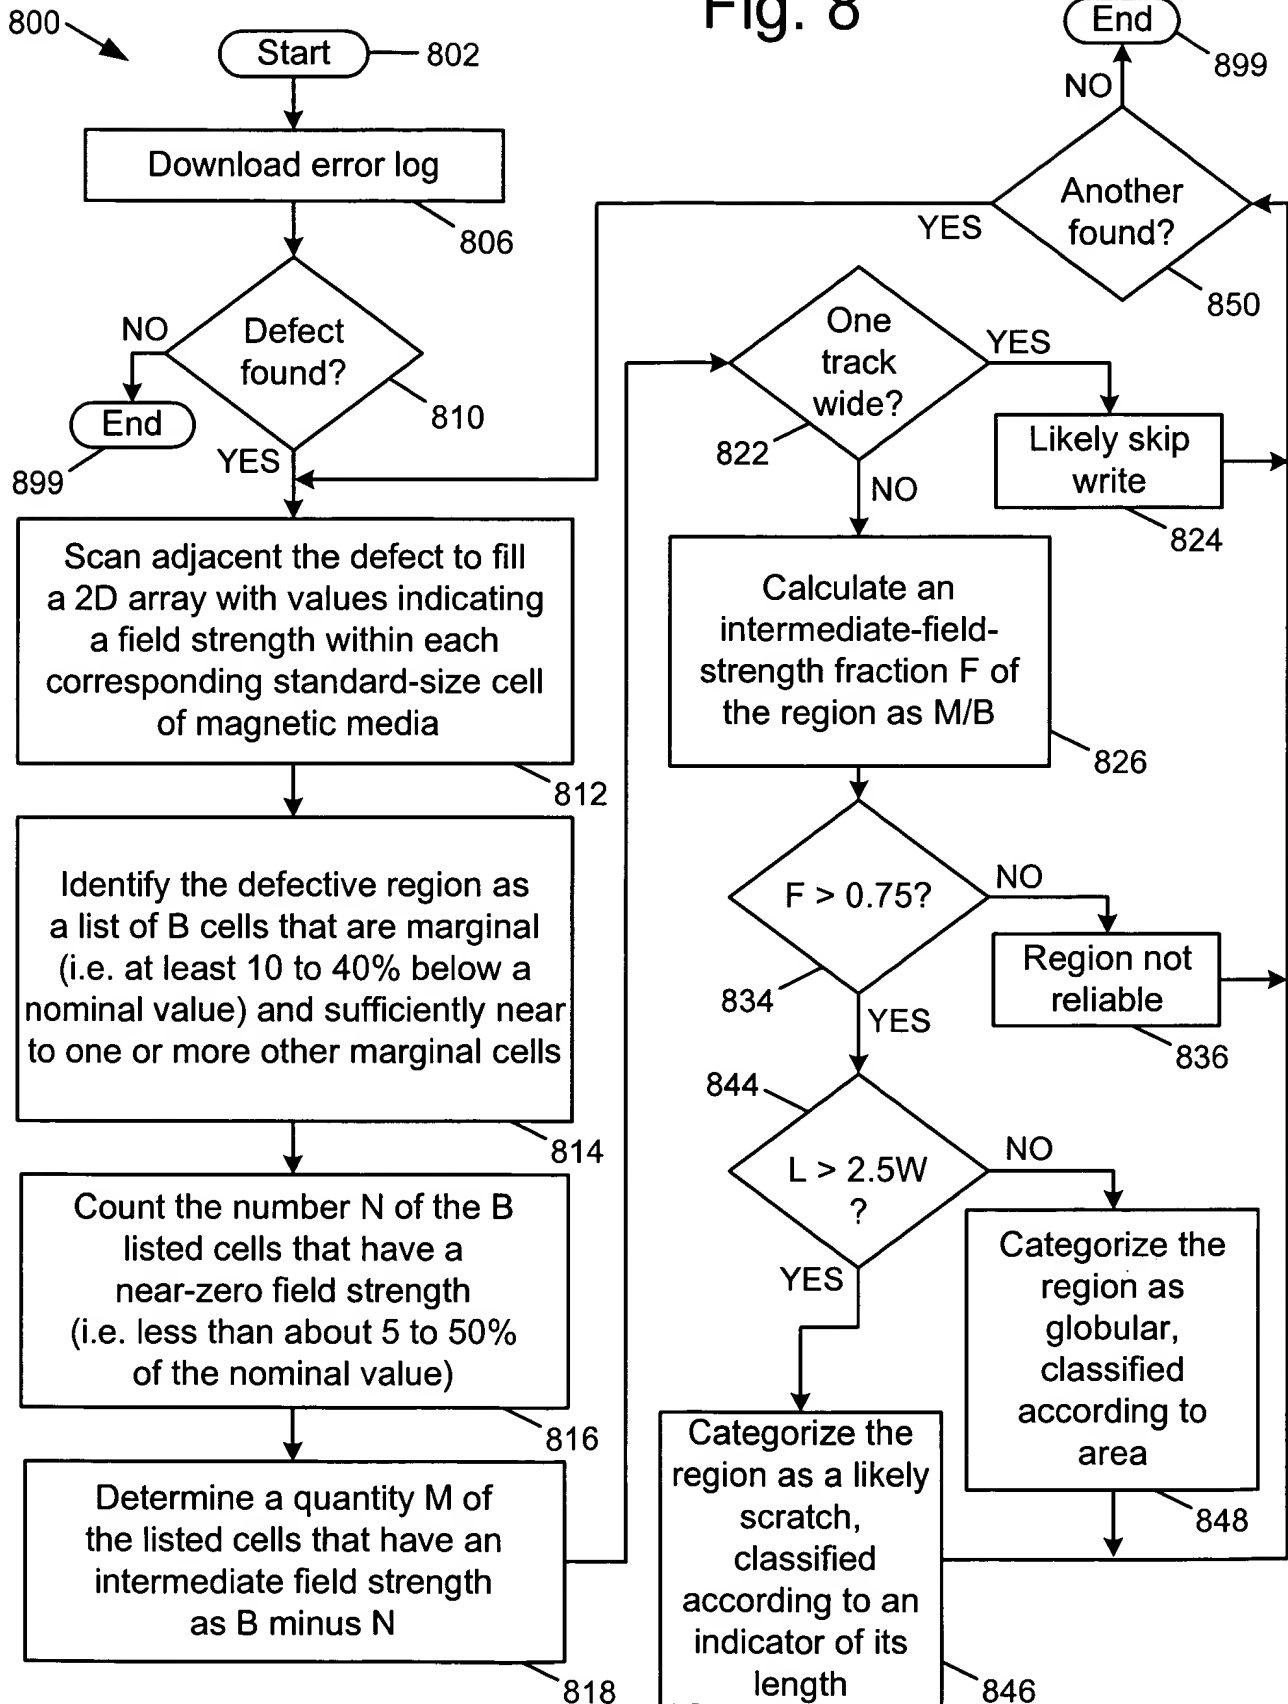

FOUO 52644660

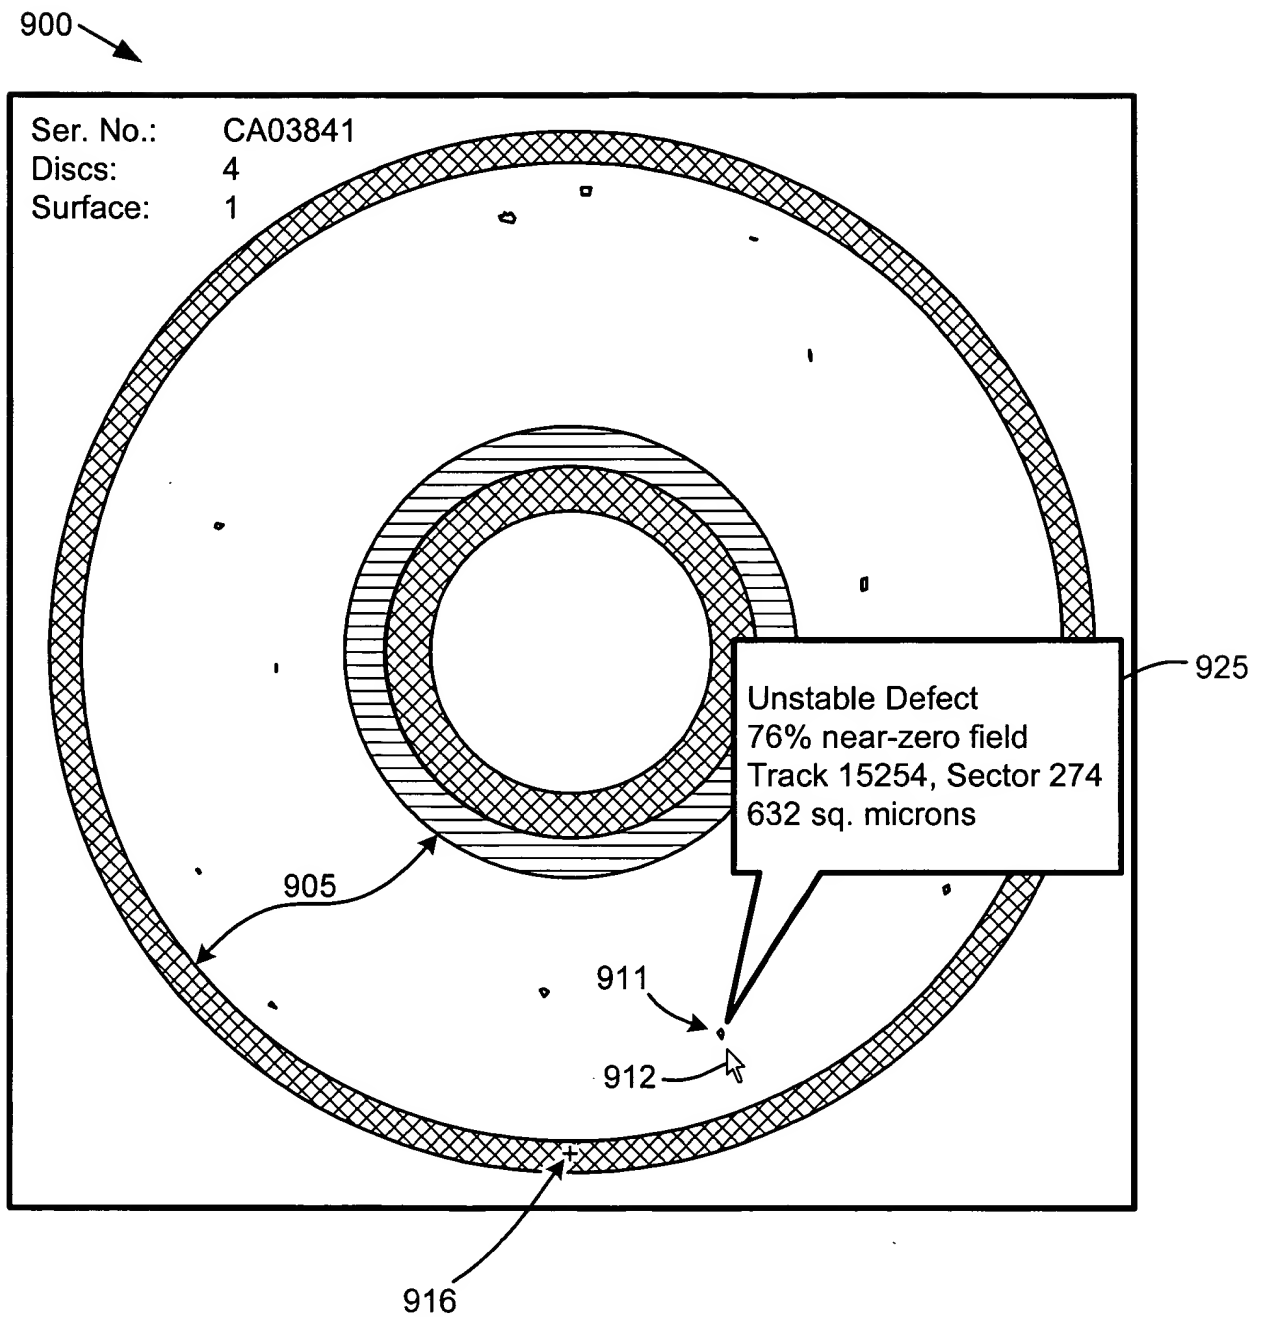


Fig. 9

Fig. 10

FIG. 10

